

Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 8/15/2014

TLW

Instrument Serial Number: 010487 As of 15-Aug-14

Start Date	End Date	Agency Name
14-Aug-14		Falls Church PD
28-Jul-14	14-Aug-14	DFS Central Lab
12-Mar-13	28-Jul-14	Richmond PD
06-Feb-12	12-Mar-13	DFS Central Lab
01-Apr-11	06-Feb-12	Prince William County PD
21-Apr-09	01-Apr-11	DFS Central Lab
07-Nov-08	21-Apr-09	Brunswick County SO
19-May-08	07-Nov-08	DFS Central Lab

INTOX EC/IR II
Quality Assurance Worksheet

HMS
TLW

Instrument Serial Number **010487** Worksheet Start Date **8/14/2014**
Location **Falls Church Police Department**
Address **300 Park Ave., Falls Church, VA 22046**
DFS Technician **Heather Stanton** License No. **18910**

☐ Laboratory

☒ On-Site

Site Specification: No detrimental environmental conditions exist. ☒

Instrument Barometer (mm HG) **751** Reference Barometer (mm HG) **751**
Reference Barometer(RB)Serial # **009113** RB Calibration Due **4/28/2015**

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.304
0.300	0.296	0.287	0.304	Sample 2	0.303
Precision		sample min	sample max	Sample 3	0.302
0.002		0.302	0.304		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.099
0.100	0.099	0.096	0.102	Sample 2	0.099
Precision		sample min	sample max	Sample 3	0.099
0		0.099	0.099		

Dry gas standard Lot No. (with tank no.) **AG419702-43**

☐ Replaced dry gas standard (+O-ring)


☒ Installed at Location

☐ Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

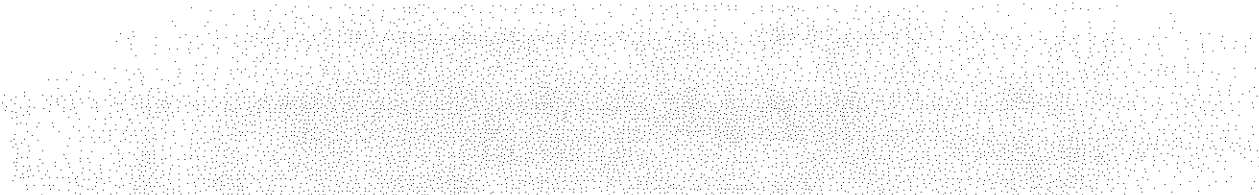

Instrument Serial Number

010487

Certification Date

☐ Calibrated☐ Certified☒ Measurement Assurance Check☒ Instrument Test☐ Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	


Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section


DFS Technician



Date

8/15/14

Issuing Analyst



Date

8/18/14

MMB

4/11/15
TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010487 Test Number: 1958

Test Date: 08/14/2014 Test Time: 12:50 EDT

Dry Gas Target: 0.296

Lot Number: AG334603-06 Exp Date: 12/12/2015

Tank Pressure: 144 psi Barometric Pressure: 751 mmHg

System Check: Passed

Test	g/210L	Time
BLK	0.000	12:50
CHK	0.304	12:51
BLK	0.000	12:53
CHK	0.303	12:54
BLK	0.000	12:55
CHK	0.302	12:56

Test Status: Success

Calibration CRC: AF74C041

HMS
TWN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010487 Test Number: 1959

Test Date: 08/14/2014 Test Time: 13:00 EDT

Dry Gas Target: 0.099

Lot Number: AG419702-43 Exp Date: 07/16/2016

Tank Pressure: 1115 psi Barometric Pressure: 751 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	13:00
CHK	0.099	13:01
BLK	0.000	13:03
CHK	0.099	13:03
BLK	0.000	13:05
CHK	0.099	13:05

Test Status: *Success*

Calibration CRC: AF74C041

HLW
TLW




COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
---	-----------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY STANTON, HEATHER, M		AGENCY DFS Central Lab
DFS LICENSE NUMBER 18910	LICENSE EXPIRES 10/01/2014	DATE TEST CONDUCTED 08/14/2014
TEST EQUIPMENT NUMBER 010487		

RESULTS: TIME SAMPLE TAKEN 13:13 EDT
 SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

☐ I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____
 SUBJECT'S SIGNATURE

☐ SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____
 OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 15 Aug 2014 at 08:25

TLN

Test Results

Instrument Serial Number 010487

Test # 001960 Subject Test

Test Location 1 Department of
Test Date 14 Aug 2014

Test Location 2 Forensic Science
Test Time 13:07
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name STANTON
Agency DFS Central Lab

Operator's First Name HEATHER

Operator's Middle Initial M

Card Serial Number 118910

License Number 18910

Effective Date 10/01/2012

Expiration Date 10/01/2014

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 14 Aug 2014 End Time 13:15

Result Time 13:13

Result Date 14 Aug 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 13:07

Data Type BLK

Sample Value 0.000

Sample Time 13:08

Data Type CHK

Sample Value 0.099

Sample Time 13:09

Data Type BLK

Sample Value 0.000

Sample Time 13:10

Data Type SUBJ

Sample Value 0.000

Sample Time 13:11

Data Type BLK

Sample Value 0.000

Sample Time 13:11

Data Type SUBJ

Sample Value 0.000

Sample Time 13:13

Data Type BLK

Sample Value 0.000

Sample Time 13:14

Standard Type Dry Gas Std

Standard Value 0.099

Standard Lot Number AG419702-43

Standard Expiration Date 07/16/2016

Tank Pressure 1115

Barometric Pressure 751 mmHg

Blow Sample Number 1 Blow Duration 3.45 sec

Blow Volume 1720 cc End-of-Blow Time 13:11

Blow Sample Number 2 Blow Duration 3.32 sec

Blow Volume 1779 cc End-of-Blow Time 13:13

Tamper Evident Stamp 7380400e

Test Status Code 0

Test Status Success